

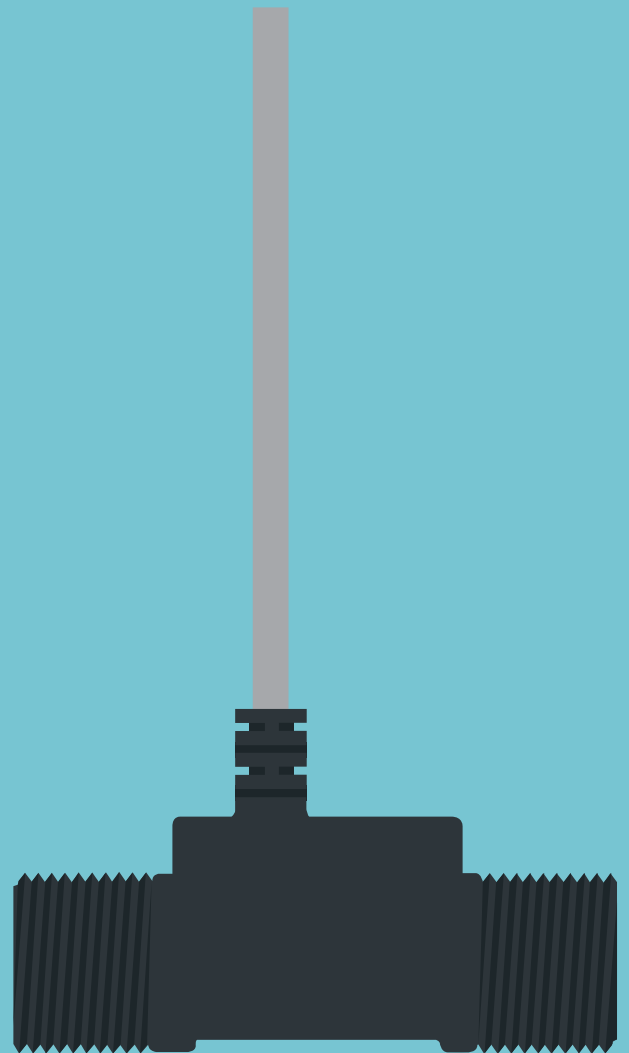
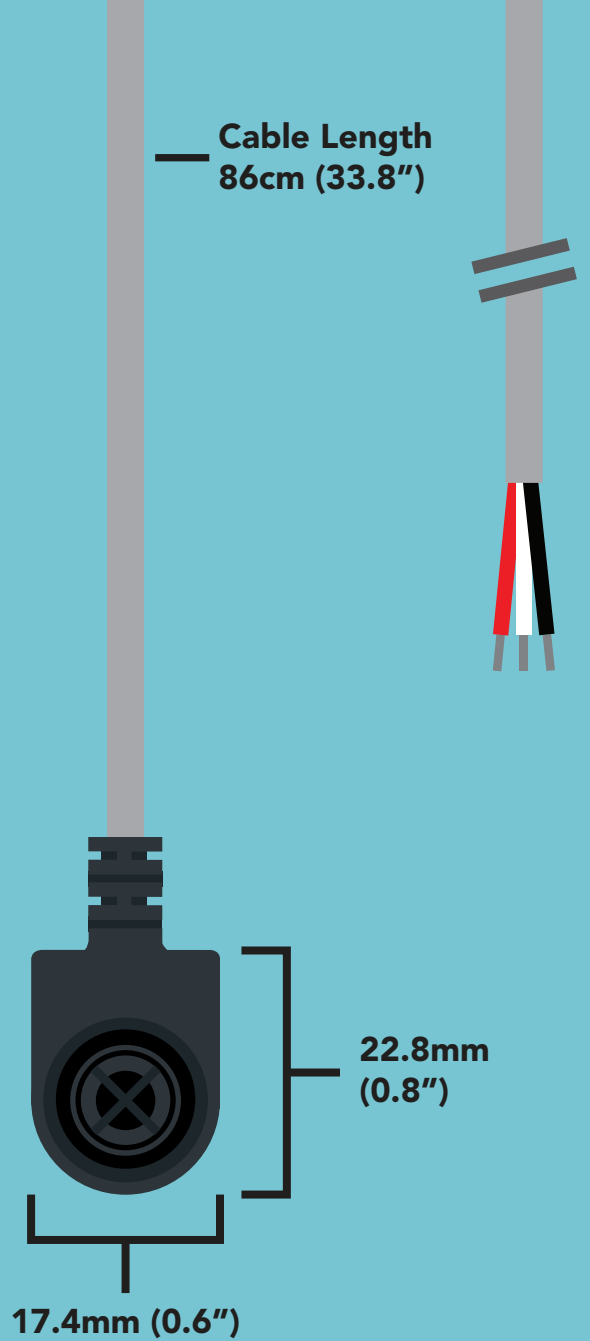


3/8" Flow Meter

Reads	Total flow and flow rate
Range	760 ml/min – 7.6 L/min
Accuracy	+/- 2%
Connector	Tinned leads
Thread	3/8" Male NPT
Max pressure	200 PSI
Temperature range °C	-20 – 80 °C
Max viscosity	81 SSU
Cable length	86cm (33.8")
Voltage	3.3V – 24 VDC
Life expectancy	~10 years

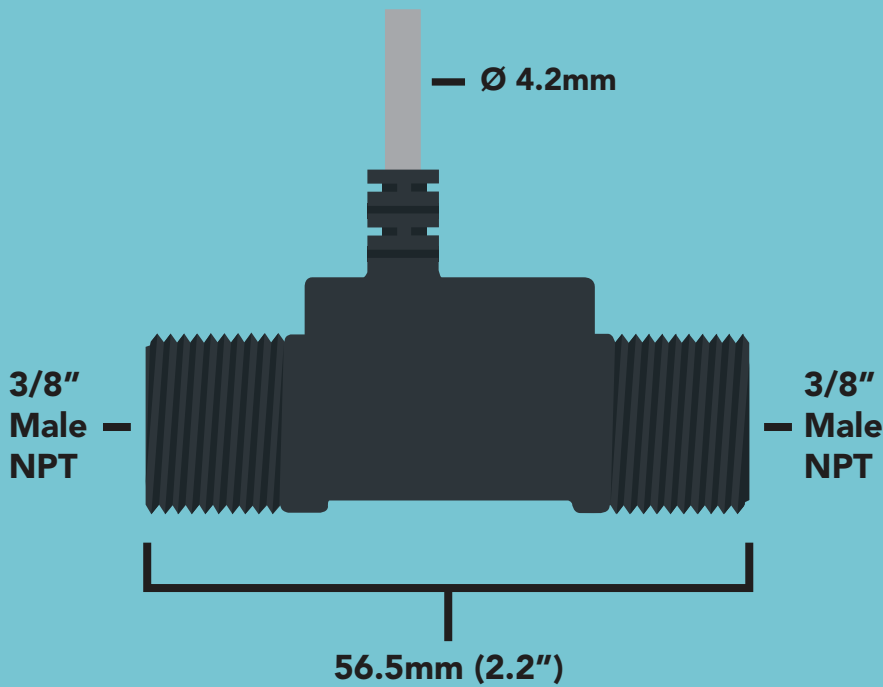


Measurements

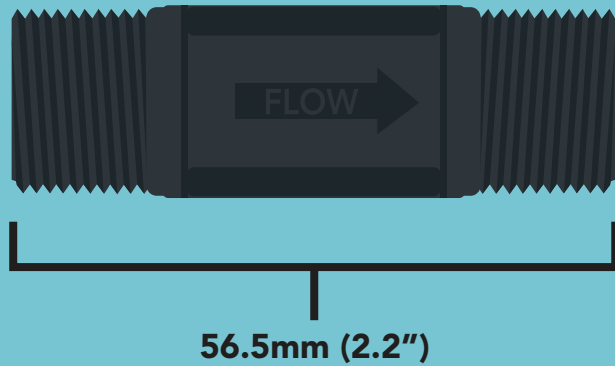

! WARNING !

**REVERSING THE POLARITY
WILL DESTROY FLOW METER.**

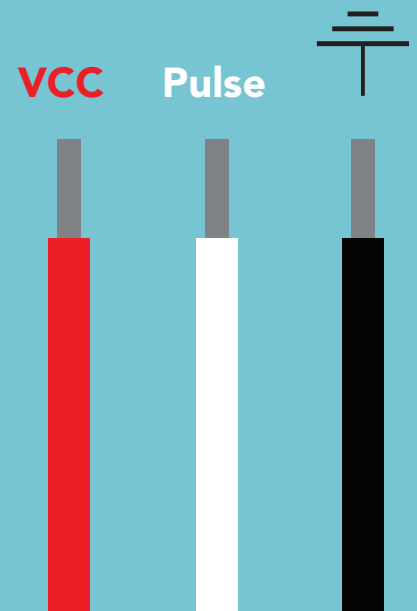

Wiring

The Atlas Scientific 3/8" Flow Meter has an 86cm (33.8") cable that terminates with three tinned leads; Red (VCC), White (Pulse), and Black (Ground). It's very important that you do not reverse the polarity or you will destroy the flow meter.

⚠ WARNING ⚠


**REVERSING THE POLARITY
WILL DESTROY FLOW METER.**

Lead Color	Function
RED	VCC 3.3V – 24V
White	PULSE
BLACK	GND

Current consumption no load 8mA
Max current consumption 25mA

VCC and PULSE must be connected together with a 10K Pull up resistor.

Microcontroller

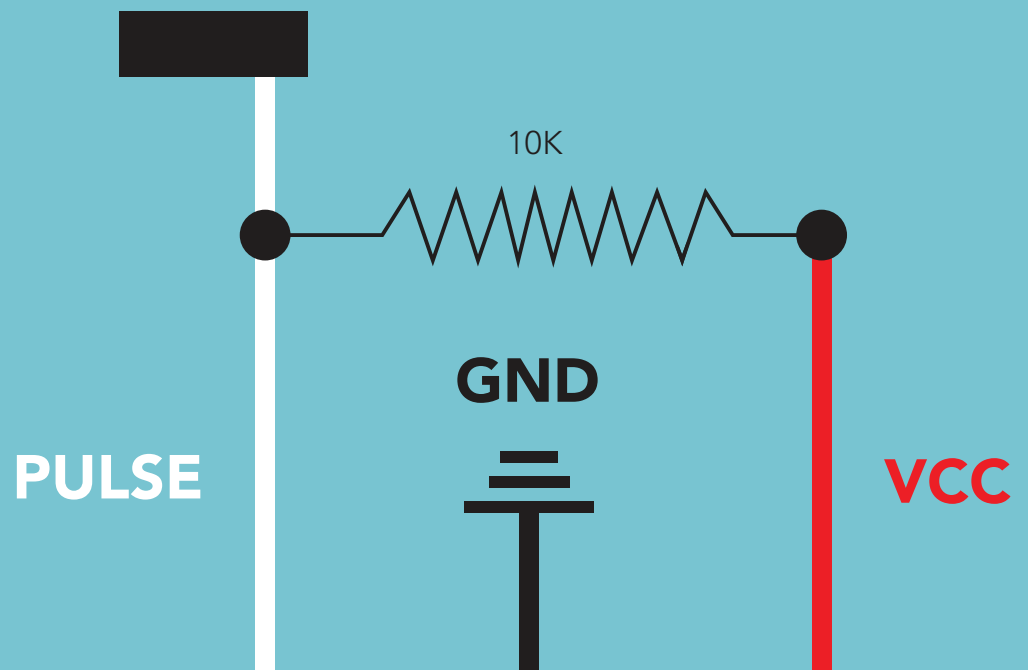

Specifications


Each rotation	367 μL
Max pressure	200 PSI
Max viscosity	81 SSU
Cable length	86 cm
Weight	101.5 grams
Food Safe	Yes
Gasoline Safe	Yes
Diesel Safe	Yes
Kerosene Safe	Yes

NSF/ANSI 61 Compliant

Atlas Scientific LLC, hereby certifies that,

**3/8" Flow Meter
Part # Sen-206F**

Complies with NSF/ANSI Standard 61

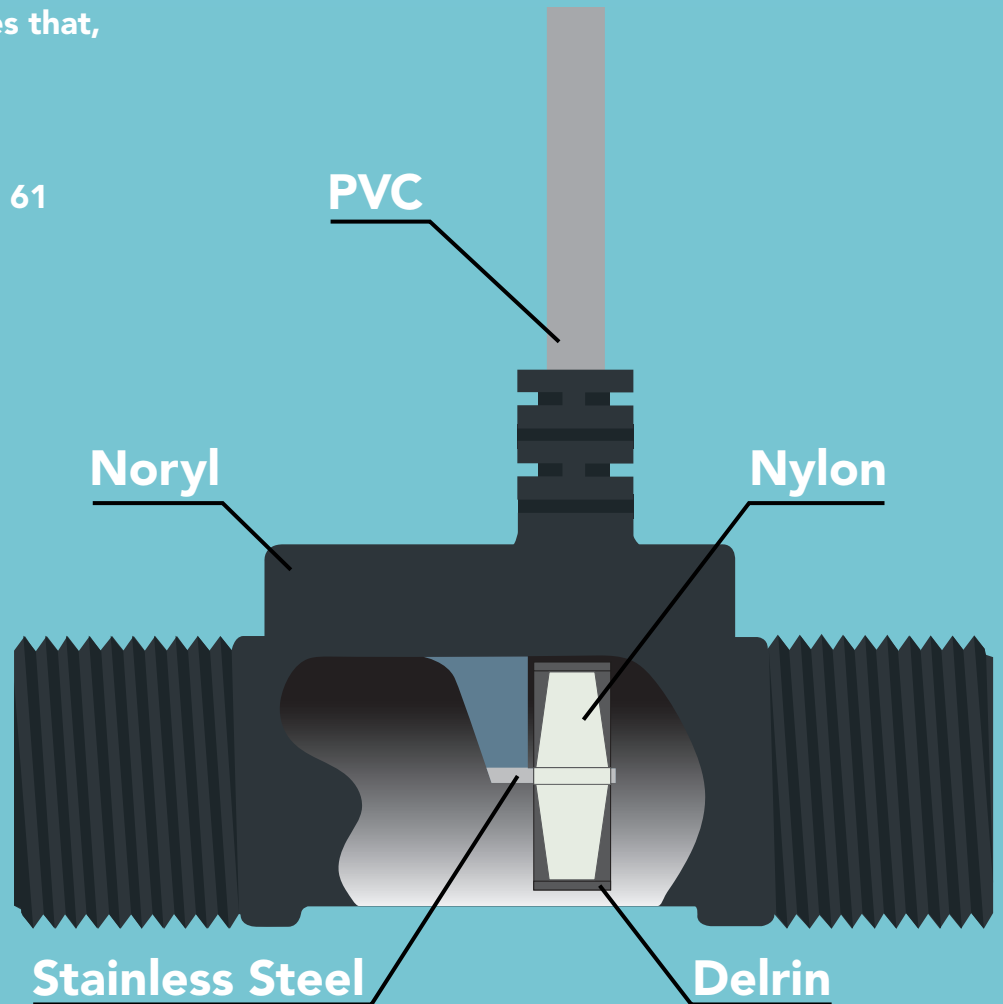

✓ **PVC**
NSF-61 Compliant

✓ **Delrin**
NSF-61 Compliant


✓ **Noryl**
NSF-61 Compliant

✓ **Nylon**
NSF-61 Compliant

✓ **Stainless Steel**
NSF-61 Compliant

Operating principle


Generally speaking, turbine flow meters are the simplest to work with and offer the highest accuracy. With this type of flow meter, each rotation of the turbine represents a volume of liquid passing through the meter.

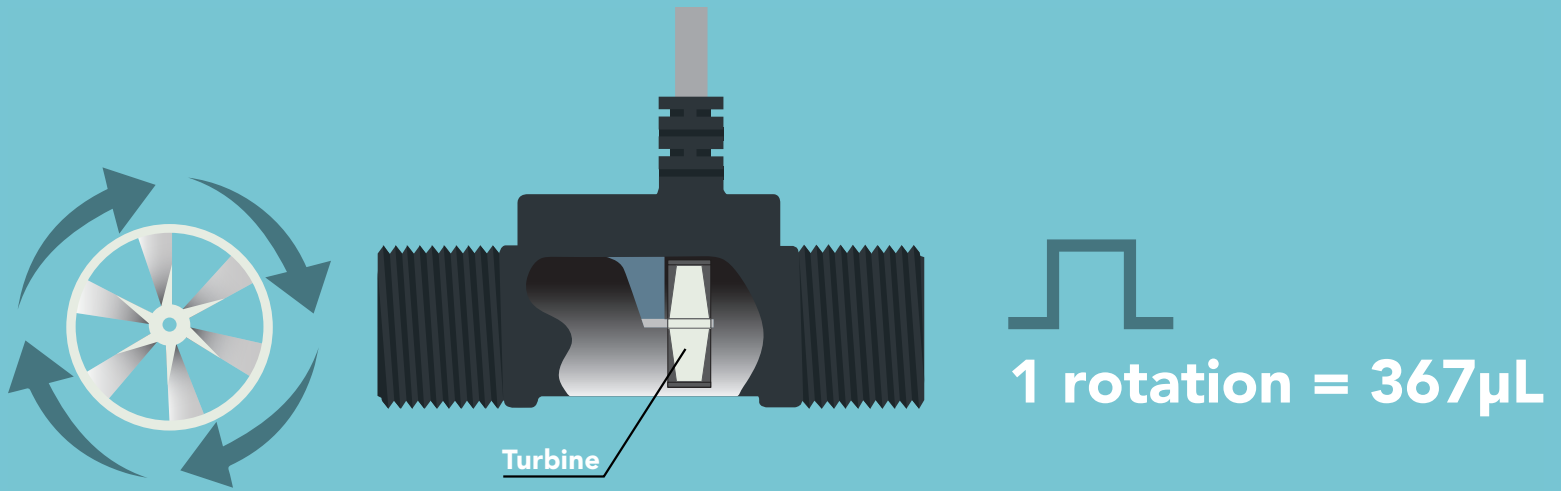

Although these flow meters are highly accurate and easy to work with, they are only cost-effective in small sizes. This flow meter is intended for low flow ranges from 760 mL/min (0.2GPM) up to 7.6 L / min (4 GPM).

Pre-filter requirements

If water with particulate matter will be passing through the flow meter, a pre-filter of at least **80 microns** must be used. Without the use of a pre-filter, the turbine blades can become jammed. Jammed turbine blades will not damage the flow meter; however, it will not be possible to get accurate flow readings until the blockage has been cleared.

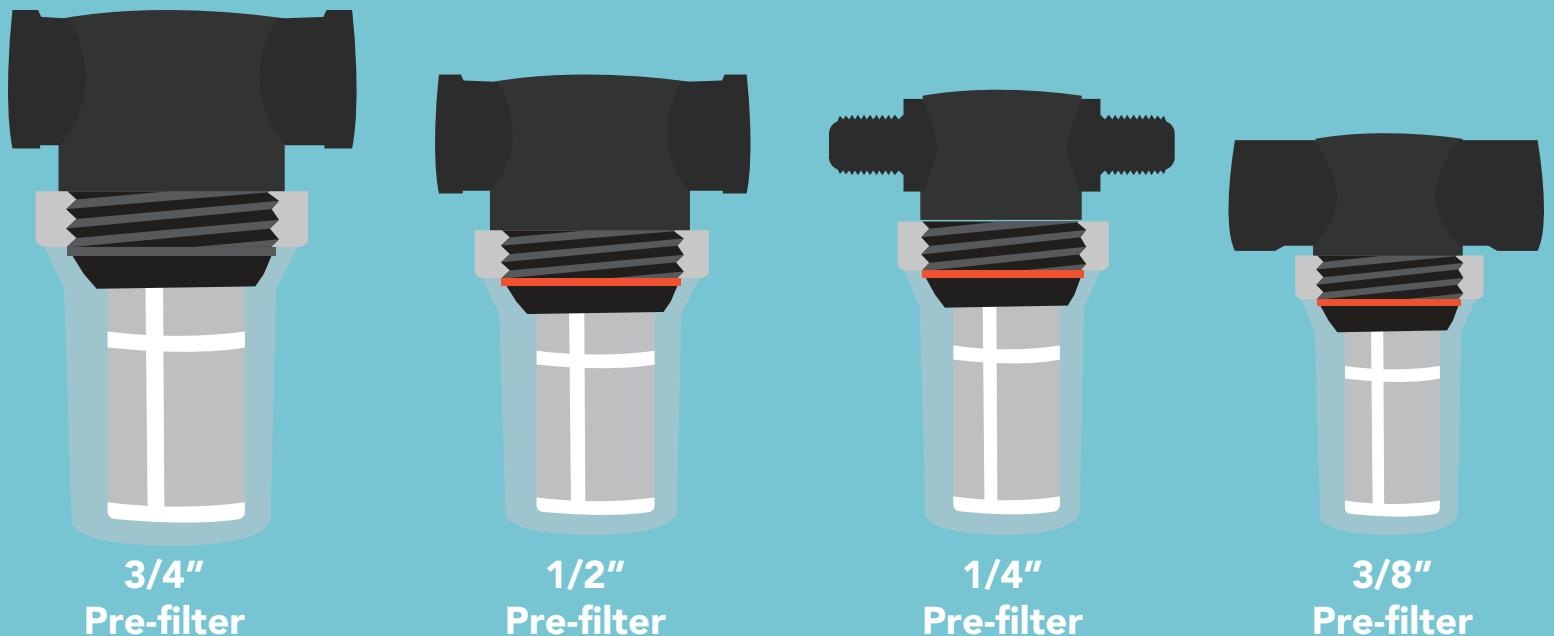

Laminar flow


Laminar flow can be thought of as the opposite of turbulent flow. In order for the flow meter to work properly, the liquid entering the flow meter should have a streamlined laminar flow. Achieving laminar flow is not hard to do; simply allow for 20cm (8") of straight pipe just before the liquid enters the flow meter.

Turbulent fluid entering the flow meter can cause inaccuracies in flow rate monitoring.


20cm (8")



Laminar flow

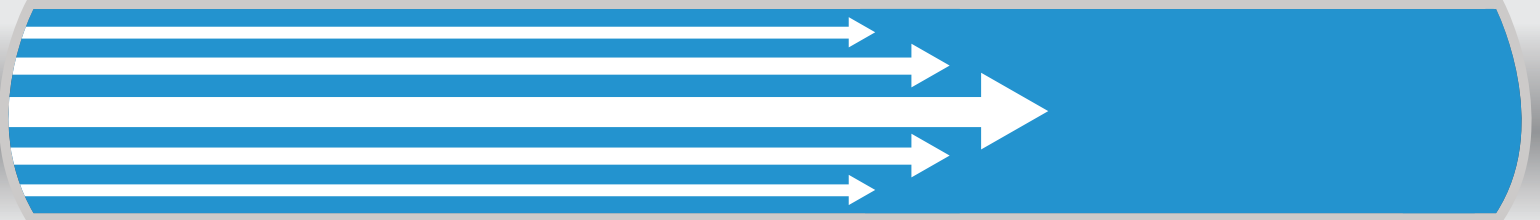


Turbulent flow

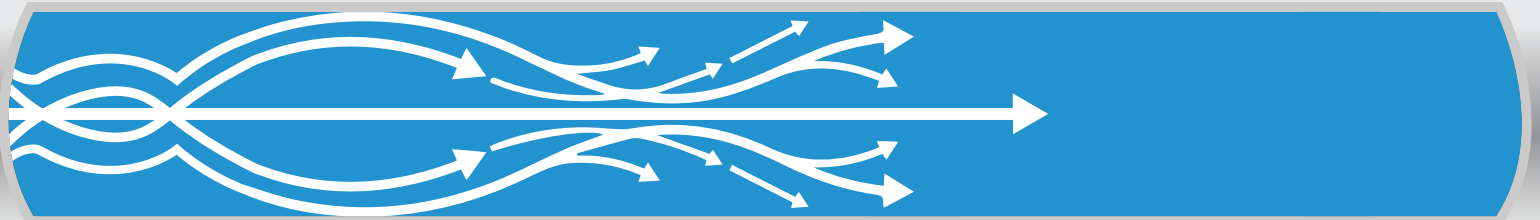

Liquid exiting the flow meter


Liquid should not be permitted to simply fall out of the flow meter. This would let air enter the flow meter and lead to inaccurate readings.

Air

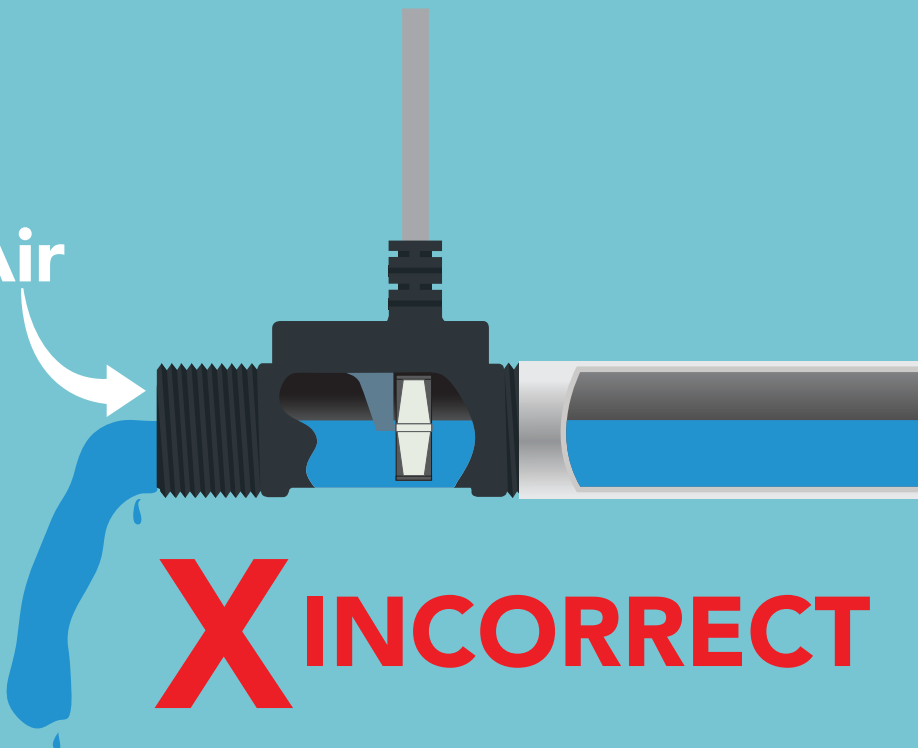

**FOR ACCURATE READINGS,
YOU CANNOT HAVE AIR IN
THE LINE.**


X INCORRECT

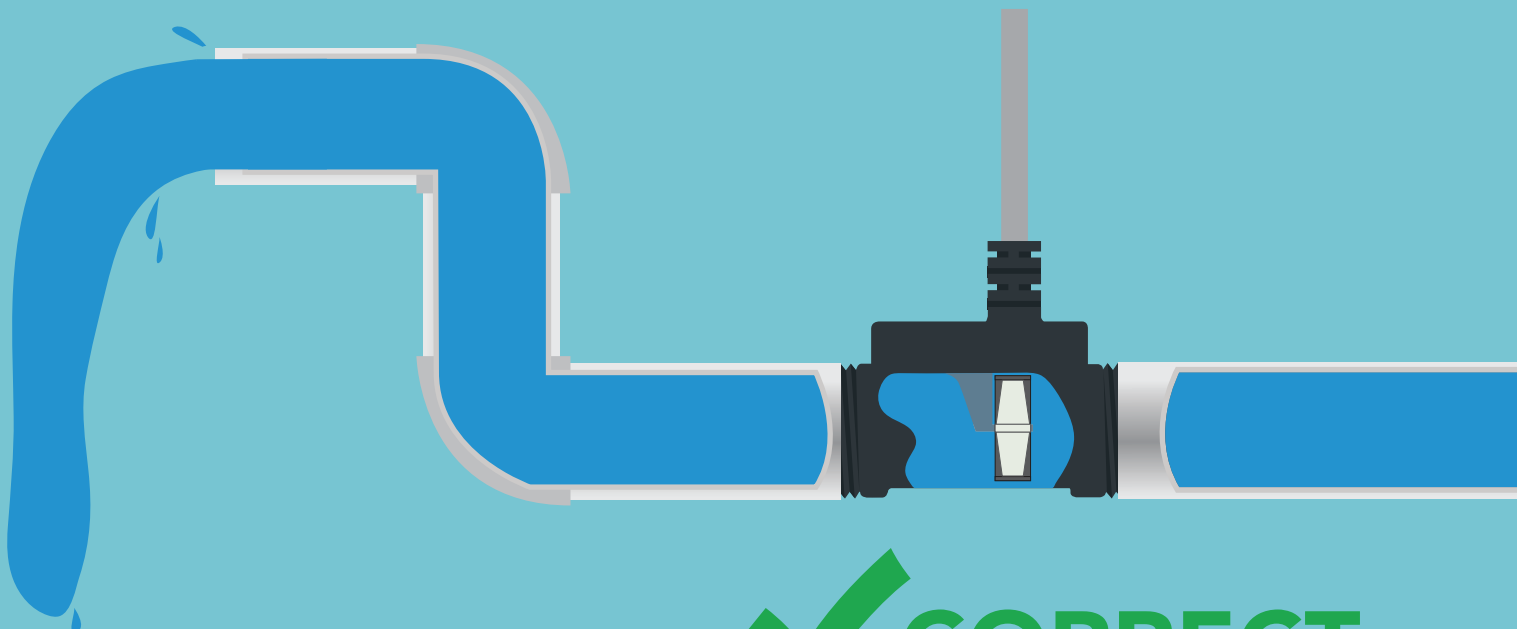

✓ CORRECT

K-factor

As stated earlier, each rotation of the turbine within this flow meter represents a volume of liquid passing through the meter. In this case each rotation is equal to 367 μ L. This flow meter is intended for low flow ranges from 760 mL/min (0.2GPM) up to 7.6 L / min (4 GPM).

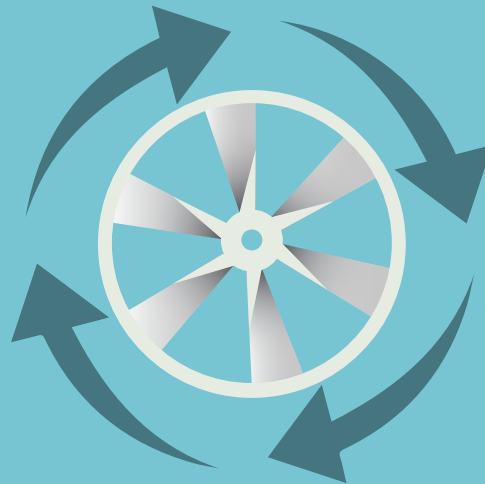

1 rotation = 367 μ L

3 rotations = 1.1mL

2,724 = 1Liter

10,313 = 1 Gallon